

Nuts and Bolts of Bubble Nasal CPAP

Jen Wung, MD, FCCM Professor-Emritus of Pediatrics of Pediatrics Columbia University Medical Center



Disclosures

Off-Label Usage: None

Interests: None


C P A P

Continuous Positive Airway Pressure

- To a spontaneous breathing patient, a positive pressure is applied to the airways throughout the respiratory cycle
- Nasal CPAP has been used at Columbia University NICU since 1973 for over 30,000 infants

CPAP Effects

- 1. Increases transpulmonary pressure and functional residual capacity (FRC)
- 2. Prevents alveolar collapse, decreases intrapulmonary shunt and improves lung compliance
- 3. Conserves surfactant
- 4. Prevents pharyngeal wall collapse
- 5. Stabilizes the chest wall
- 6. Increases airway diameter and splints the airways
- 7. Splints the diaphragm
- 8. Stimulates growth of the immature lung
- Bubble CPAP has HFV effect/stochastic resonance

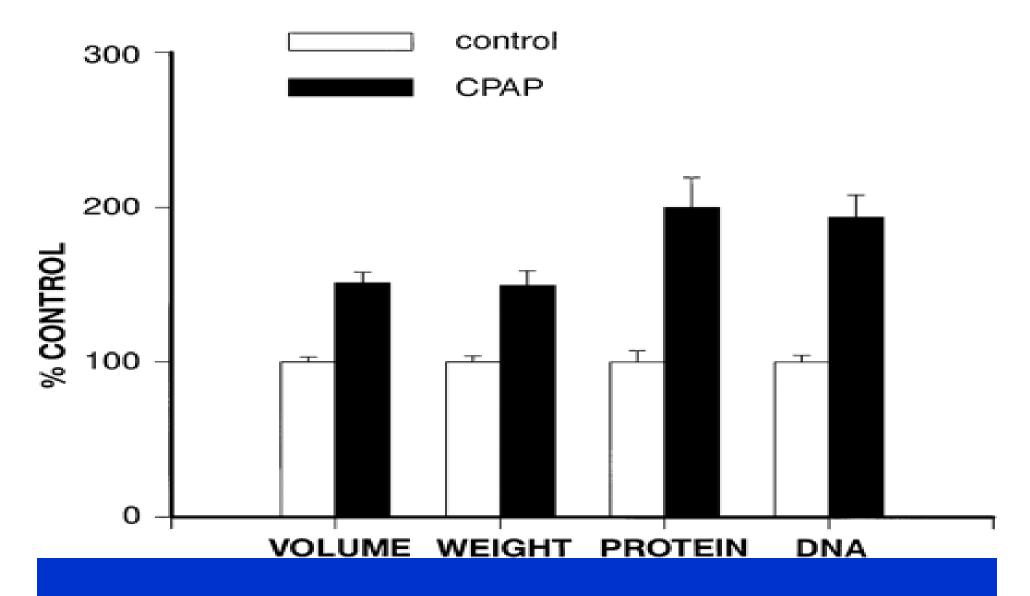


Lung volume, lung weight, and protein and DNA contents at end of study were higher in CPAP-exposed than in control animals (all P < 0.01). Strain-induced growth of the immature lung. Zhang S. et al. J. Appl Physiol 1996;81:1471-6

Premature baby Surfactant Structural deficiency lung (RDS) immaturity

CPAP


- CPAP is not just for RDS
- CPAP stimulates the growth of the immature lung
- keeping the premature infants on CPAP, even on room air CPAP, as long as they are symptomatic (e.g., tachypnea, retraction or apnea & bradycardia.)

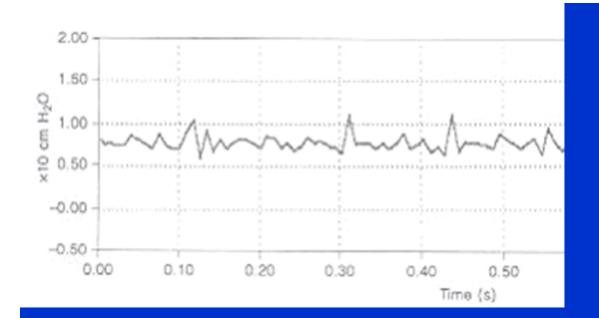

Waveform produced at airway with underwater **Bubble CPAP**

Amplitude 2-4 cm H2O, Frequency 15-30 Hz

Lee K-S et al: Biol Neonate 73: 69-75, 1998

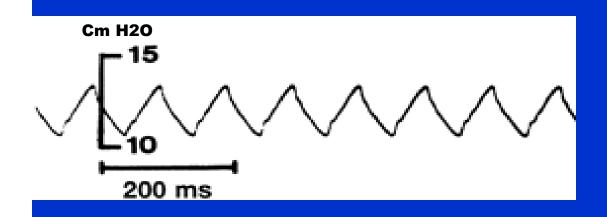

Waveform produced at airway with <u>HFOV</u>
(Sensormedics)

Set I-time 0.3 Set Frequency 10 Hz


Thome U: J Appl Physiol: 84(5):1520-7, 1998

C P A P

Indication


- 1. Diseases with low FRC, e.g. RDS, TTN, PDA, pulmonary edema, etc.
- 2. Apnea and bradycardia of prematurity
- 3. Meconium aspiration syndrome (MAS)
- 4. Airway closure disease, e.g. bronchiolitis, BPD
- 5. Tracheomalacia
- 6. Partial paralysis of diaphragm
- 7. Respiratory support after extubation

Effect of alveolar radius and surface tension on alveolar stability w/ and w/o surfactant Law of LaPlace P = 2 T/r

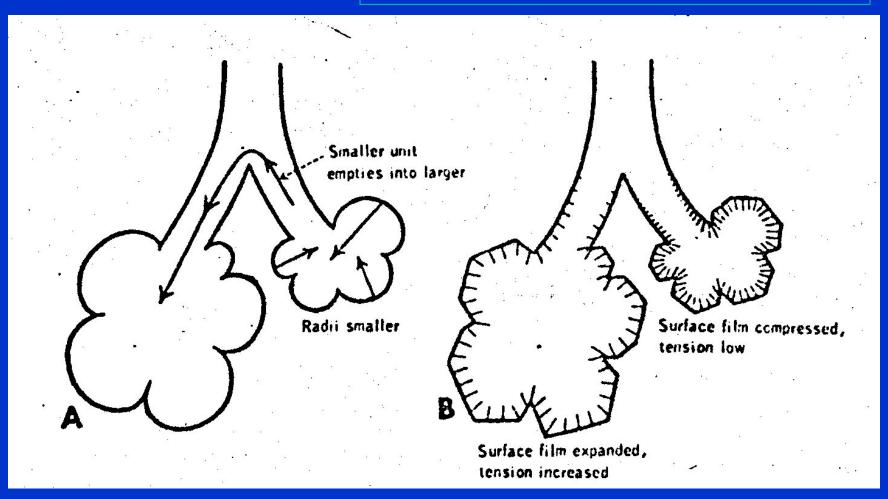


Law of LaPlace : P = 2T/r

P: pressure T: surface tension r: radius

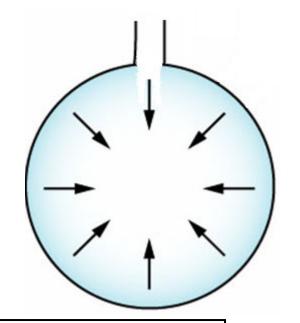





Larger alveolus

$$r = 2$$
$$T = 3$$

$$P = (2 \times 3) / 2$$

$$P = 3$$

Smaller alveolus


$$r = 1$$

$$T = 3$$

$$P = (2 \times 3) / 1$$

$$P = 6$$

Natural response of surfactant producing cells to birth Spain CL et.al. Ped. Research, 1987

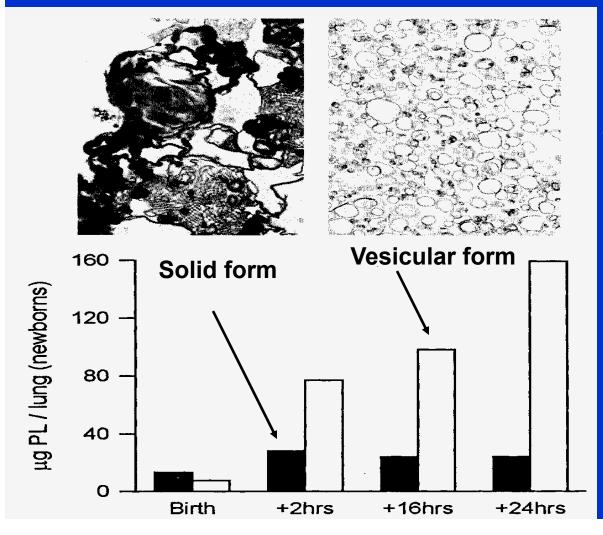


At onset of breathing, amount of surfactant pool increases significantly


C P A P

Indication


- 1. Diseases with low FRC, e.g. RDS, TTN, CPIP, PDA, pulmonary edema, etc.
- Apnea and bradycardia of prematurity
- Meconium aspiration syndrome (MAS)
- 4. Airway closure disease, e.g. bronchiolitis, BPD
- 5. Tracheomalacia
- 6. Partial paralysis of diaphragm
- 7. Respiratory support after extubation

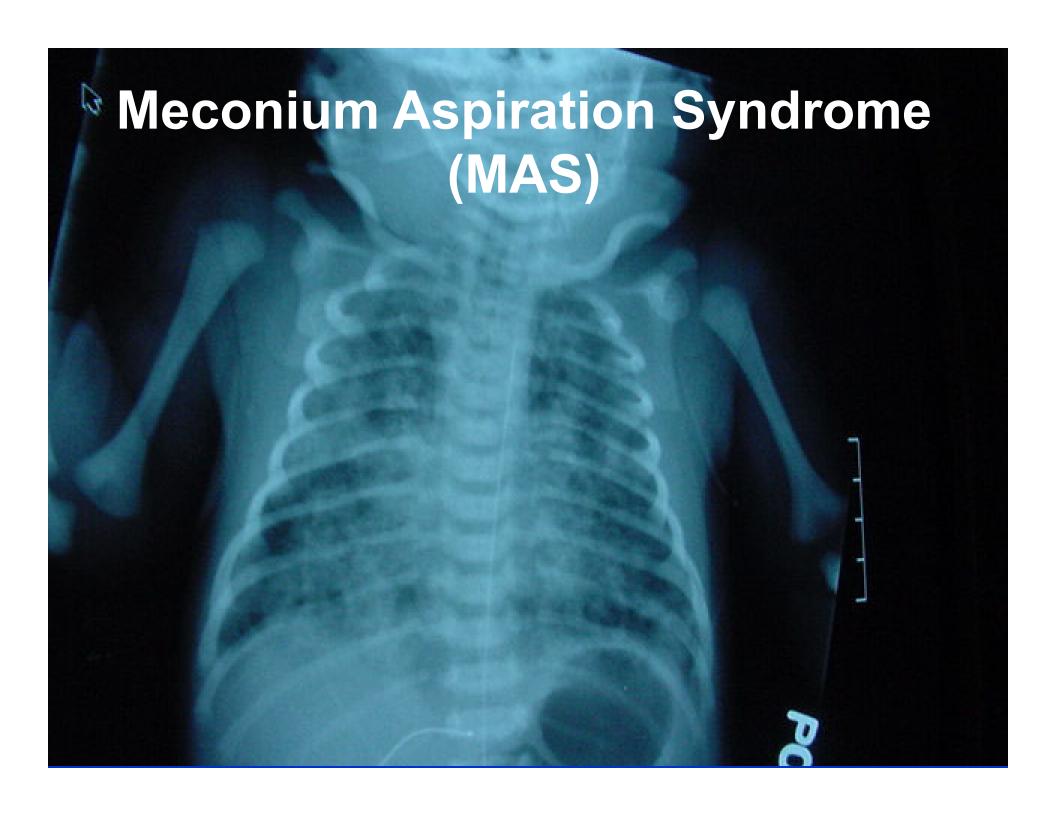


Meconium Aspiration Syndrome (MAS)

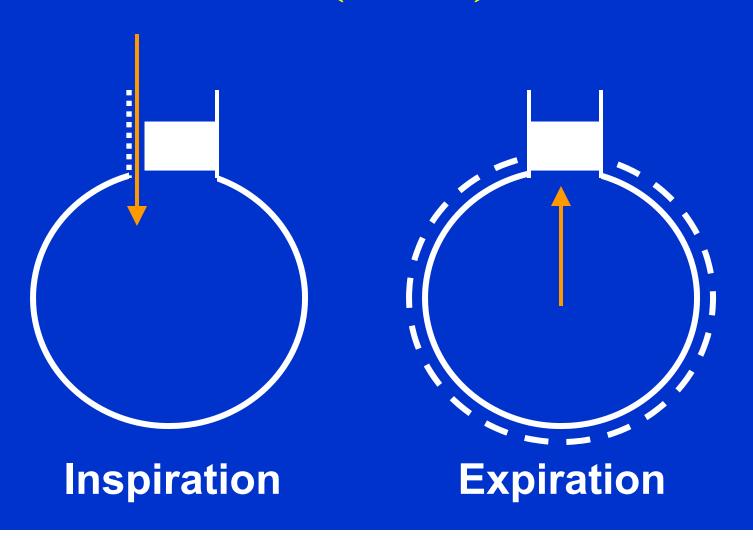

Meconium Aspiration Syndrome (MAS)

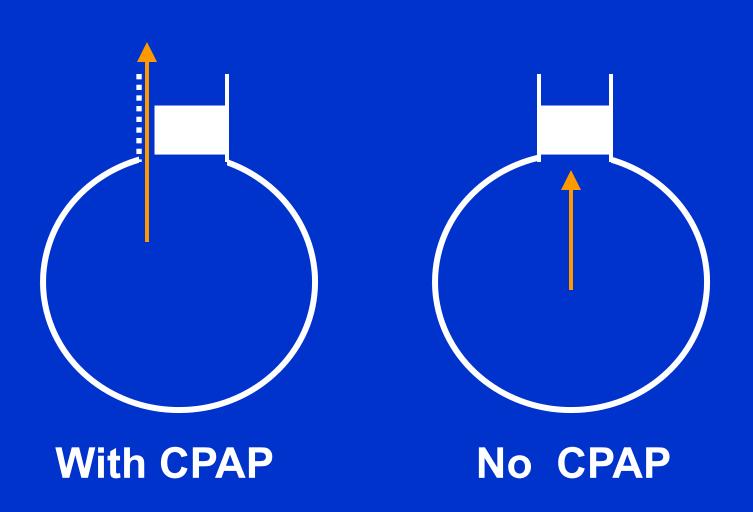

Waterfall Effect

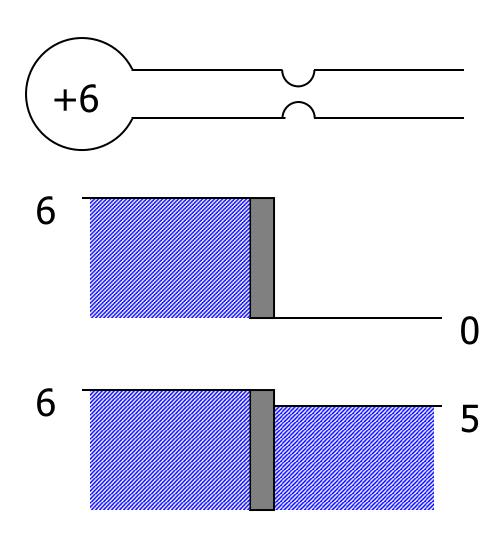



C P A P

Indication

- 1. Diseases with low FRC, e.g. RDS, TTN, CPIP, PDA, pulmonary edema, etc.
- 2. Apnea and bradycardia of prematurity
- 3. Meconium aspiration syndrome (MAS)
- Airway closure disease, e.g. bronchiolitis, BPD
- Tracheomalacia
- 6. Partial paralysis of diaphragm
- 7. Respiratory support after extubation


CPAP Device

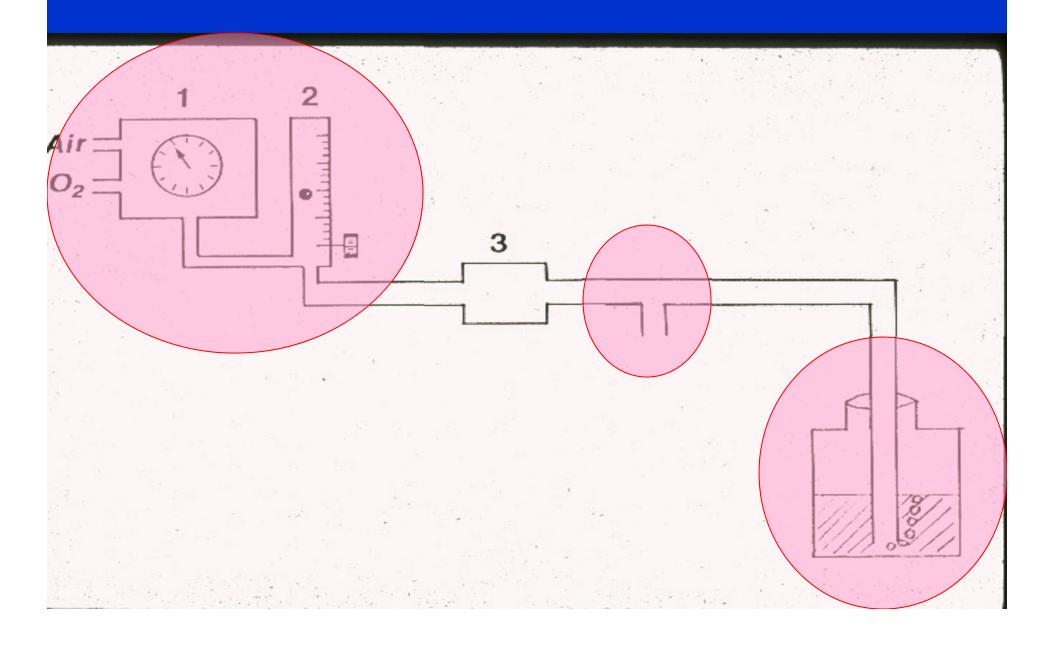


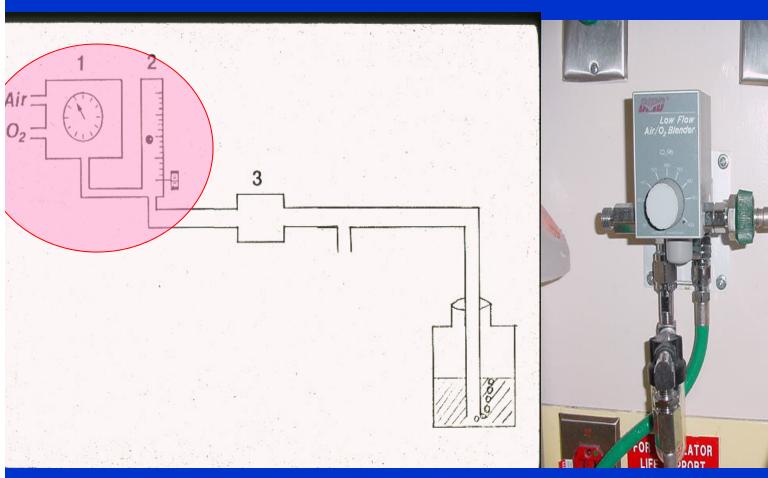






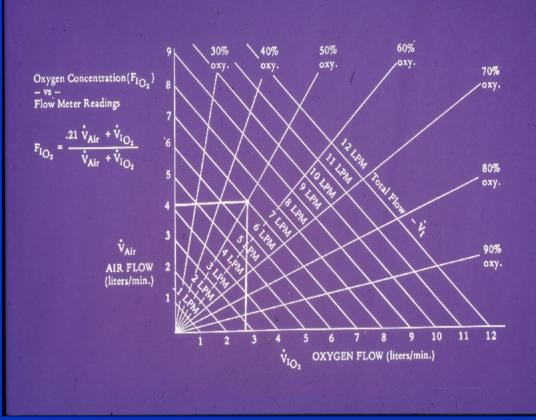


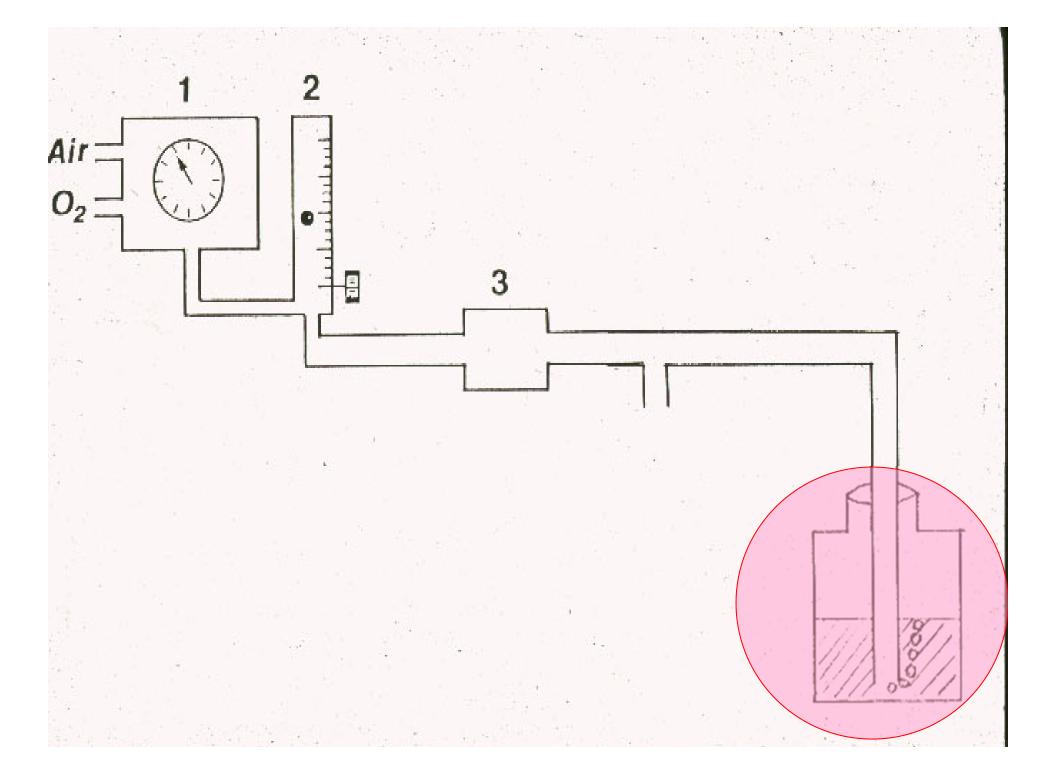


Modes of positive pressure generation

- Threshold resistors the level is determined by the force applied to the surface area of the valve. The pressure generated is independent of flow. (*Water bubble CPAP*)
- Variable pressure-flow resistors the level of PEEP/CPAP is directly proportional to the product of the gas <u>flow</u> through the orifice of the expiratory pressure valve and the <u>resistance</u> of the valve. (*Ventilator provided CPAP*)
- Variable flow- Flow opposition with fluidic flow reversal during expiration (coanda effect) (Infant flow driver)

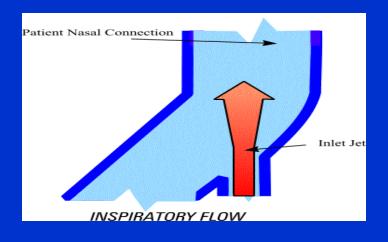


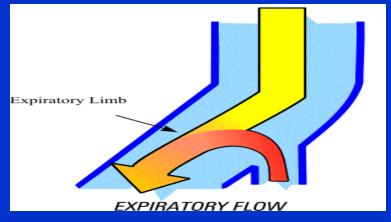


EFFECT OF ANGLE ON OSCILLATIONS

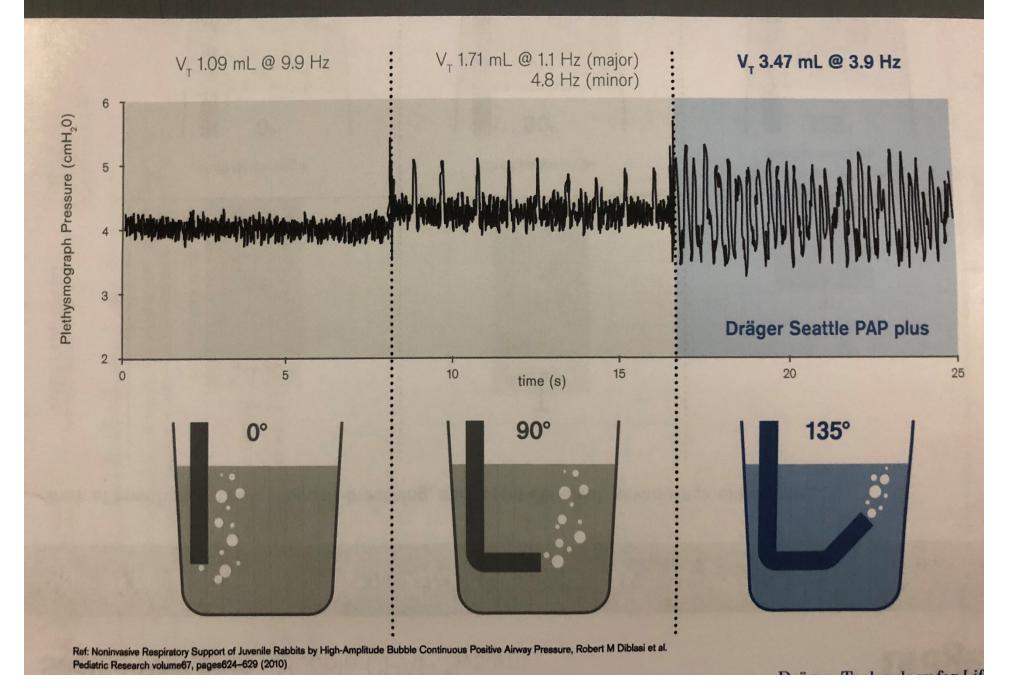

ANGLE OF BUBBLELATOR SIGNIFICANTLY REDUCES WORK OF BREATHING (WOB)



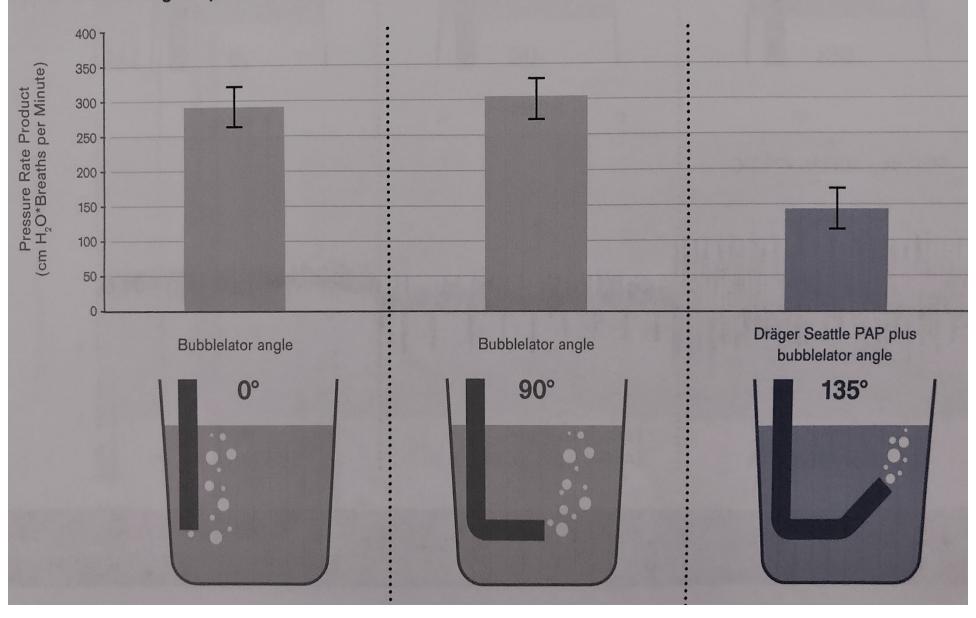

Bubble-CPAP vs Ventilator-CPAP

All infants with bubble CPAP had:

- a lower minute volume with a mean reduction in MV of 39% (p<0.001)
- 7 % reduction in respiratory rate (p=0.004)
- With no change in transcutaneous CO₂ and oxygen saturation values

Lee K-S et al: Biol Neonate 73: 69-75, 1998

Physiological Advantage of Bubble versus Ventilator-derived CPAP

- Lower PaCO₂
- Higher PaO₂, PH, FRC
- Less V/Q mismatch
- Lower alveolar protein


Bubble Continuous Positive Airway Pressure Enhances Lung Volume and Gas Exchange in Preterm Lambs

Jane Pillow et al. Am J Respir Crit Care Med. 2007; 176(1): 63-69.

B-NCPAP vs V-NCPAP

- Randomized crossover study in 18 premature infants (<1500 g) with mild respiratory distress
- Work of breathing, breathing asynchrony, respiratory rate, heart rate, tidal volume, minute ventilation, lung compliance or TcPCO₂ was not significantly different
- TcPO₂ was higher with B-NCPAP (P=0.01)

Courtney, SE et al.: Journal of Perinatology (2011) 31, 44–50;

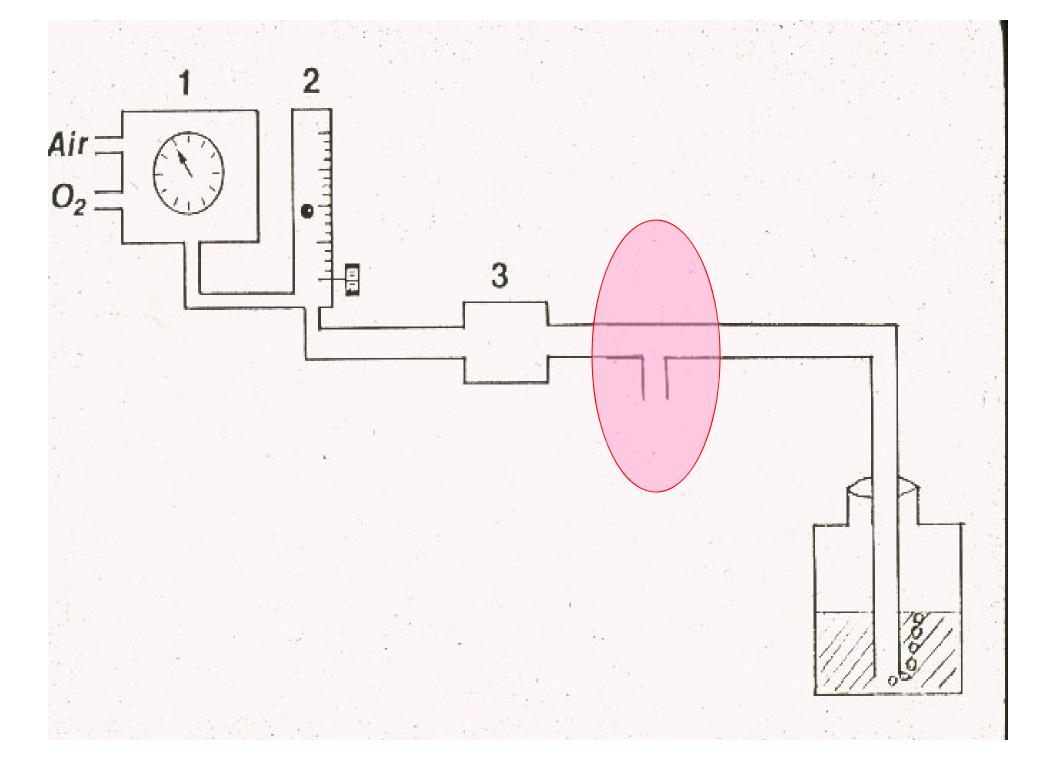


CPAP Devices (Interface)

- Head hood
- Face shield
- Face mask
- Nasal mask
- Nasal prongs Hudson, Babi-plus nCPAP
 INCA, Draeger, Fisher&Pakel, SiPAP, Arabella
 Infant Flow, NeoPAP
- Nasal cannula Vapotherm, Ram Cannula
- Nasal pharyngeal tube
- Endotracheal tube

Not all CPAP devices are created equal

There is a learning curve for CPAP therapy

CPAP was first described for use in newborn infants by Professor August Ritter von Reuss in his 1914 textbook on diseases of the newborn infant.

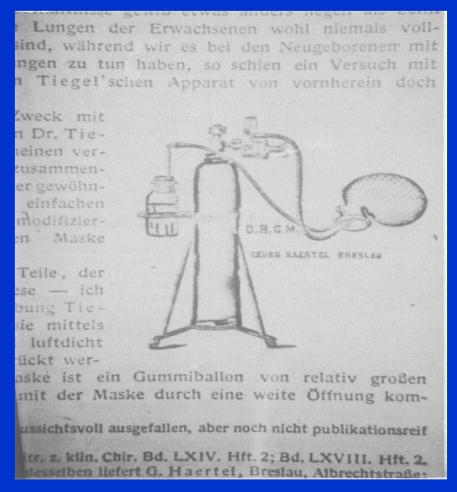


VonTiegel's over-pressure apparatus'(1911)

Treatment of idiopathic respiratory distress syndrome with continuous positive airway pressure

Weight	N	PaO ₂ (pre)	PaO ₂ (post)
930-1500	10	37.1	116.4
1501-2000	5	38.1	114.8
2001-3830	5	48.6	96.0


Gregory et al. N Engl J Med 284: 1333, 1971

Treatment of idiopathic respiratory distress syndrome with continuous positive airway pressure

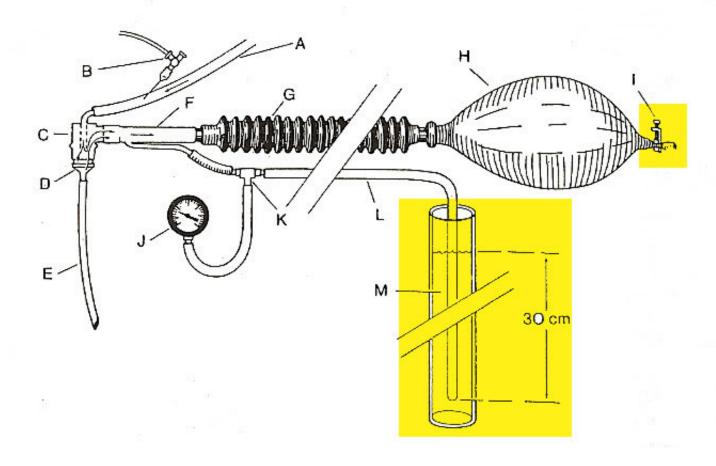



Gregory et al. N Engl J Med 284: 1333, 1971

Head Box for CPAP without Endotracheal Tube

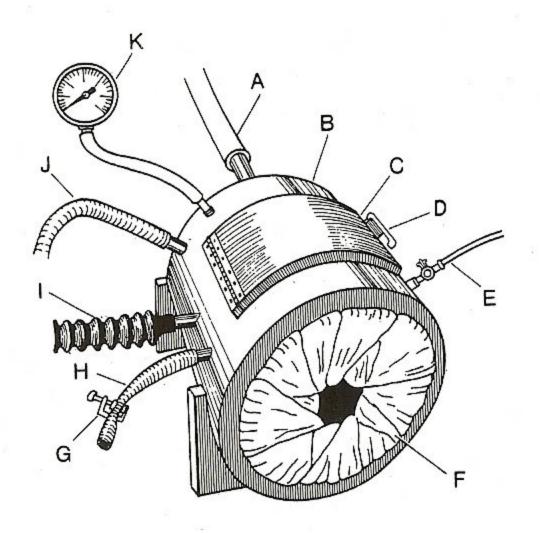



Gregory, et al., NEJM, 1971

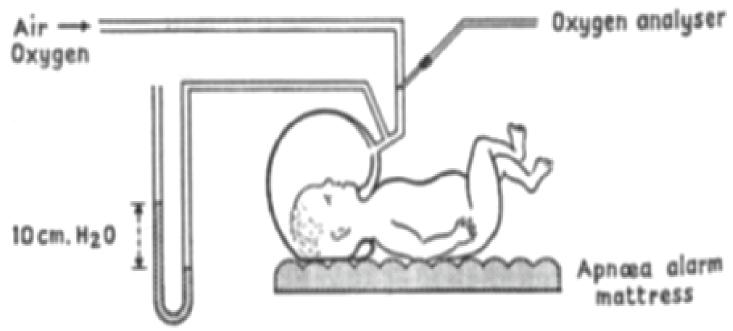


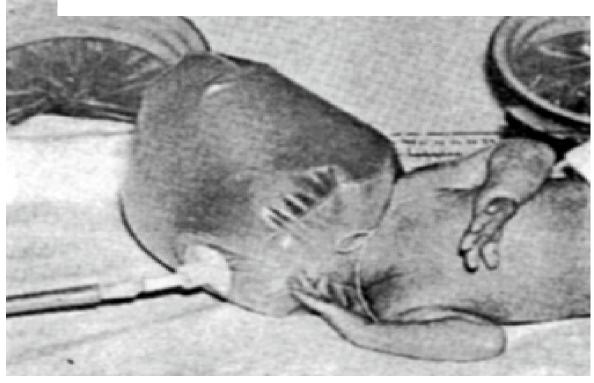

H. Barrie, Lancet, i (1972), p. 776

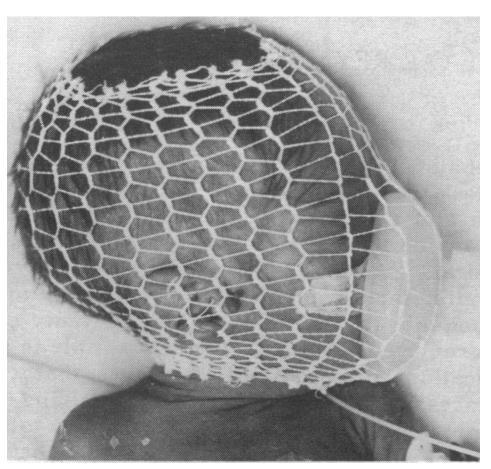

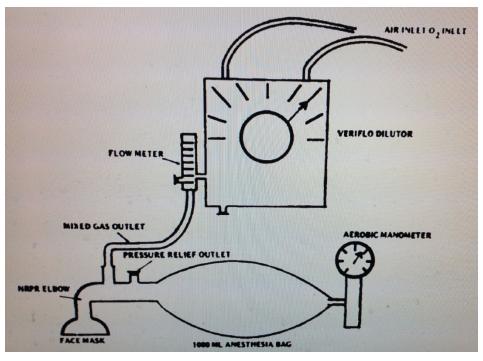

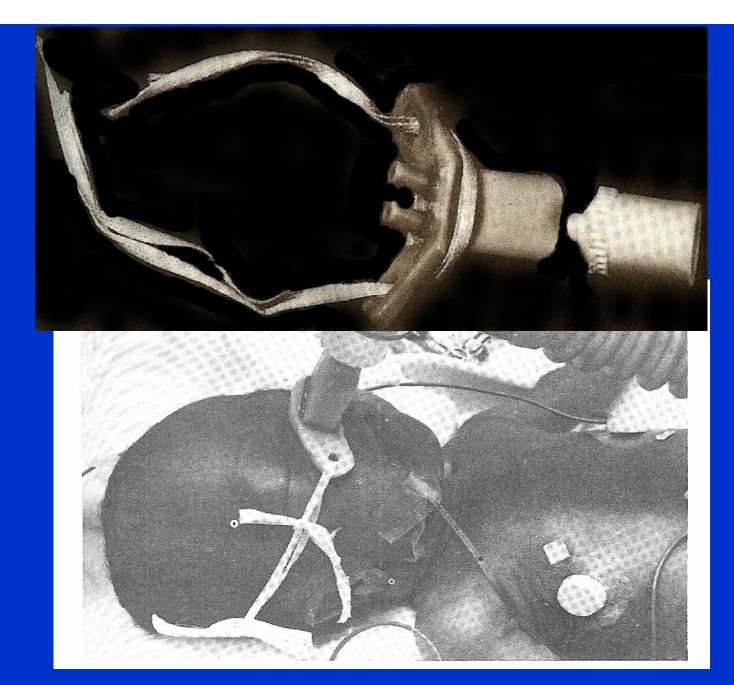


Kattwinkel, Fleming, Cha, and Fanaroff, Pediatrics, 1973;52;131







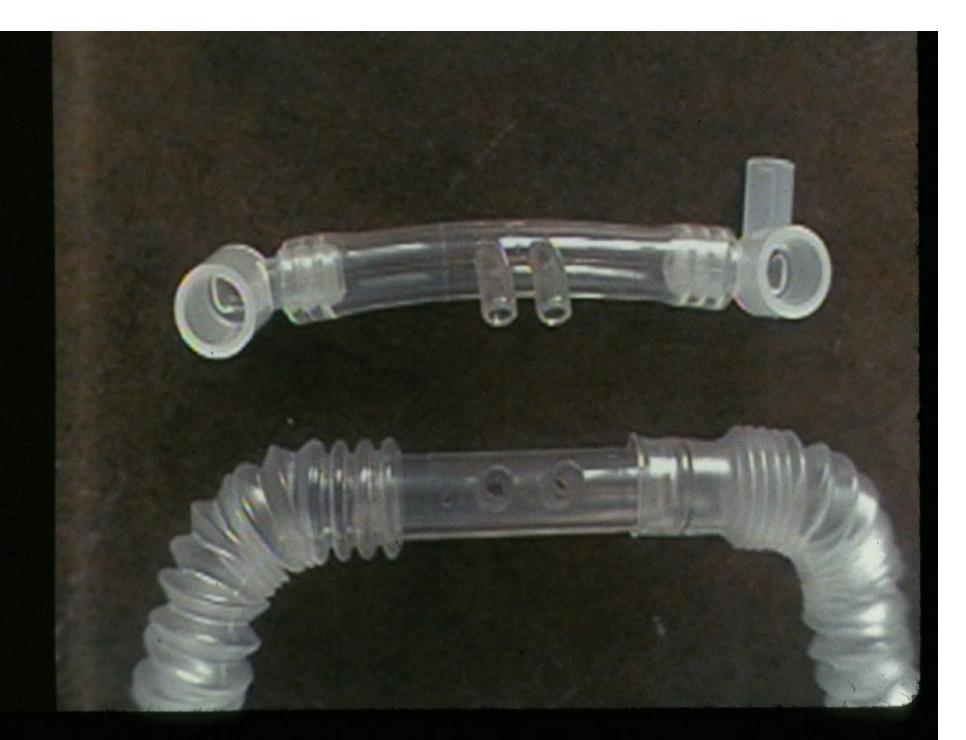

CPAP Cannulae (Hudson)



Babi-plus nCPAP Size 7 – size 0



Made of silicone, not PVC. latex-free



INFANT FLOWTM nCPAP System





Fisher & Paykel






Nasal Cannula

Nasal CPAP






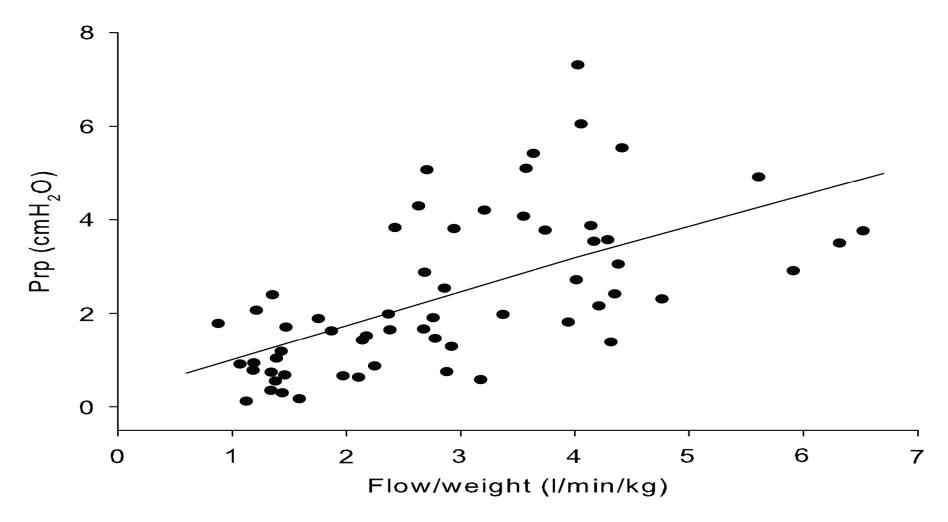

Linear regression between flow rate divided by infants'weight and end-expiratory Prp in heated, humidified, high-flow, nasal cannula (HHHFNC) (Prp=0.3+0.7*V'; r2=0.37)


Respiratory Mechanics during NCPAP and HHHFNC at equal distending pressure, Anna Lavizzari et al. Arch Dis Child Fetal Neonatal Published online 30 April 2014

Mean hypopharyngeal pressures and Gas flow in preterm infants with nasal cannula

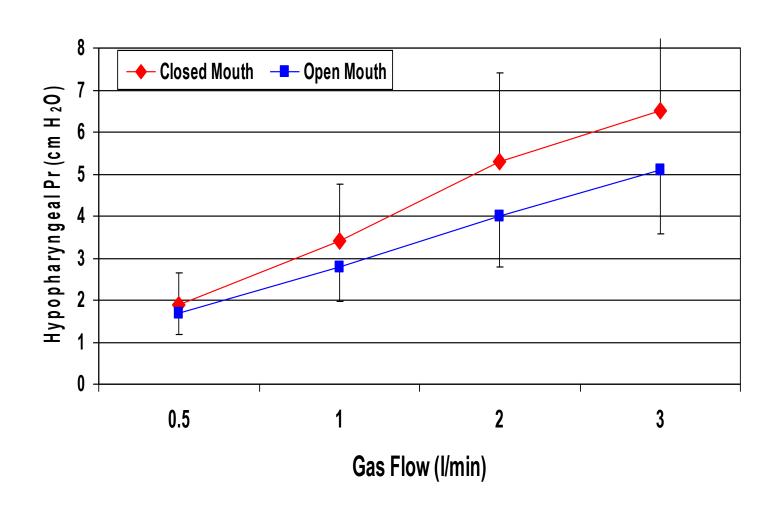



Presión Hipofaríngea en prematuros con cánula nasal: Relación con el flujo de gas

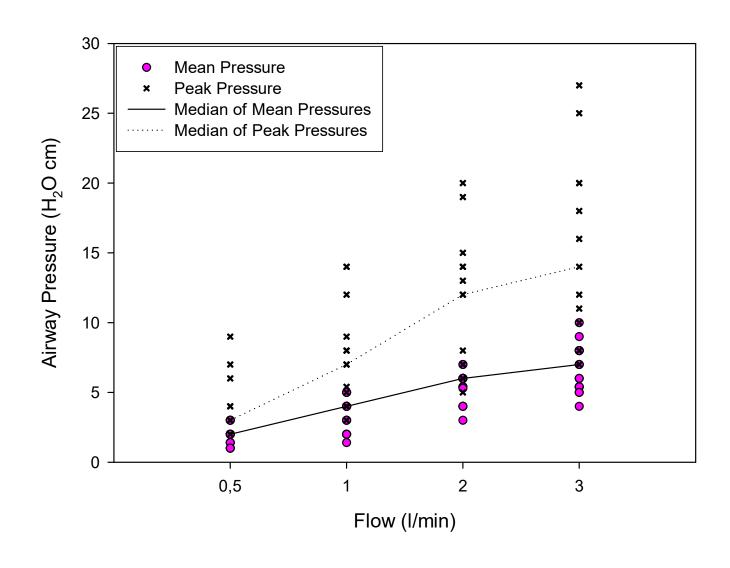

Hypopharyngeal oxygen concentration and pressure delivered by nasal cannula in preterm infants Alvaro Quintero et al. PAS 3450-3, 2009

Gas Flow	Hypopharynx FiO2	Hypopharyx Pressure
LPM	Median (Range)	Median (Range)
0.1	0.28 (0.23 - 0.42)	
0.3	0.44 (0.30 - 0.61)	
0.5	0.53 (0.37 - 0.69)	2.7(1.3-13.6)
1	0.69 (0.49 - 0.90)	4.7 (1.3 – 19)
2	0.75 (0.53 - 0.91)	5.4 (4.0 -20.4)

Subcutaneous scalp emphysema, pneumo-orbitis and pneumocephalus in a neonate on high humidity high flow nasal cannula

LR Jasin, S Kern, S Thompson, C Walter, JM Rone and MD Yohannan

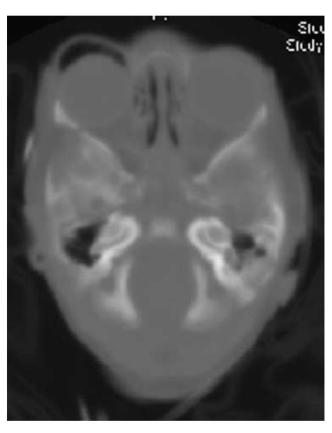


Figure 2 Computerized tomography of the head demonstrating orbital air and subcutaneous scalp emphysema.

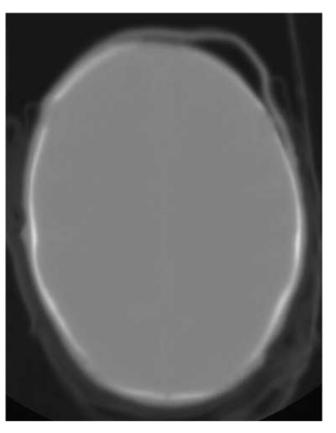


Figure 4 Computerized tomography of the head demonstrating orbital air and subcutaneous scalp emphysema.

Nasal Cannula

- •The CPAP and FiO₂ delivered will depend upon the cannula size, flow, anatomy of nose and space between cannula and nose
- No safety mechanism to assure that excessive positive pressure is not given
- •" ---High–flow nasal cannula should not be used as a replacement for delivering CPAP." Kubicka et al. Pediatrics 2008;121:82-88
- "--- easy may not be safe." –Finer, 2005

			HHHFNC	nCPAP
Collins, 2013	Extubation Failure	Total	15/67	22/65
(J Pediatr)		28-32 wk	7/37	8/36
		<28 wk	2/30	1/29
	BPD		24/67 (36%)	28/65(43%)
Manley, 2013	Extubation Failure	Total	52/152	39/151
(NEJM)		26-32 wk	26/120	20/120
		<26 wk	26/32	19/31
	BPD		47/152 (31%)	52/151 (34%)

Incidence of BPD

CHONY (6/99 - 7/02)

Proposed New Definition

BW(g)	GA(wks)	O ₂ (36 wks)	Mild	Mod.	Severe	
< 750	25.4 ± 2.0	1 8.3%	31.6%	15.0%	3.3%	
750-1000	26.9 ± 1.8	1.4%	16.9%	1.4%	0	
1001-125	$0 29.0 \pm 1.8$	3 1.1%	0	1.1%	0	
Total	27.4 ± 2.4	5.9%	14.1%	5.0%	0.9%)

Sahni et al. J Perinatol 25(1):41-6, 2005.

Reasons for different results in previous CPAP studies

- The difference in devices used and experiences of caregivers
- The difference in threshold of CPAP failure
- Studies did not show significant reduction of BPD because CPAP therapy was discontinued too early to take advantage of stimulation of lung


HFNC vs CPAP

Use of HFNC in ELBW infants is associated with:

- A higher risk of death or BPD
- Increased respiratory morbidities
- Delayed oral feeding, and
- Prolonged hospitalization.

Dalal K. Taha et.al. J Pediatr 2016;173:50-5)

CPAP Delivery System (Columbia)

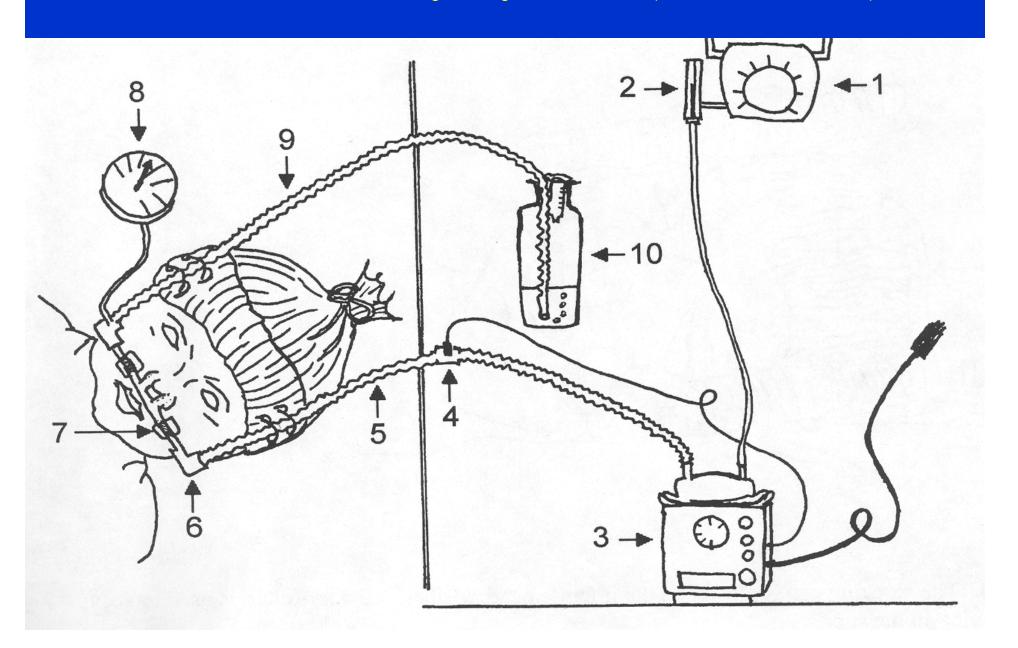


CPAP prong vs ET tube




ET tube ID:	Resistance (cmH2O/5lpm)
2.5 mm (length 10 cm)	14.2
3.0 mm (length 12 cm)	6.5
3.5 mm (length 12 cm)	4.3
Hudson CPAP prong size:	
0	2.5
1	1.0
2	1.0
3	0.5
4	0.5
5	0.5

Nasal CPAP Set up (1)

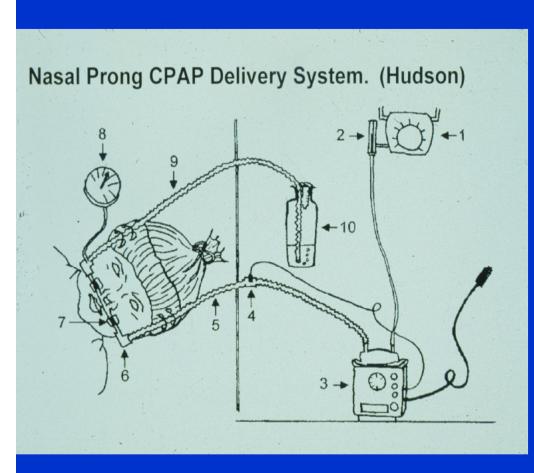

- 1. Oxygen blender
- 2. Flowmeter (5-10 LPM)
- 3. Heated humidifier
- 4. Thermometer
- 5. Inspiratory tubing
- 6. Nasal cannulae
- 7. Velcro

Nasal CPAP Set up (2)

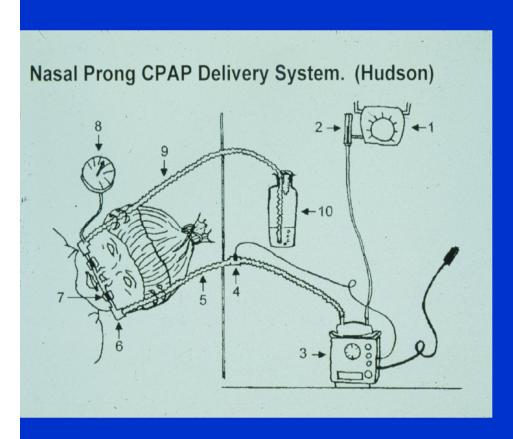

- 8. Manometer (optional)
- 9. Expiratory tubing
- 10. A bottle containing a solution of 0.25% acetic acid filled up to a depth of 7 cm. Distal tubing immersed to a depth of 5 cm to create +5 cmH₂O

Nasal CPAP Application (1)



- 1. Position the baby in supine position with the head elevated about 30 degrees
- 2. Place a small roll under the baby's neck
- 3. Put a pre-made hat or stockinet on the baby's head to hold the CPAP tubings

Nasal CPAP Application (2)



4. Choose FiO₂ to keep PaO₂ at 50's or O₂ saturation at 90 – 95%

Alarm set at 85-95%

Nasal CPAP Application (3)



- 5. Adjust a flow rate 5-10 lpm to:
- a) provide adequate flow to prevent rebreathings CO₂
- b) compensate leakage from tubing connectors and around CPAP prongs
- c) generate desired CPAP pressure (usually 5 cmH₂O)




6. Keep inspired gas temperature at 37° C

Nasal CPAP Application (5)



7. Insert the lightweight corrugated tubing (preferrably with heating wire inside) in a bottle of 0.25% acetic acid solution or sterile water filled up to a height of 7 cm. The tube is immersed to a depth of 5 cm to create 5 cmH₂O CPAP as long as air bubbling out of solution



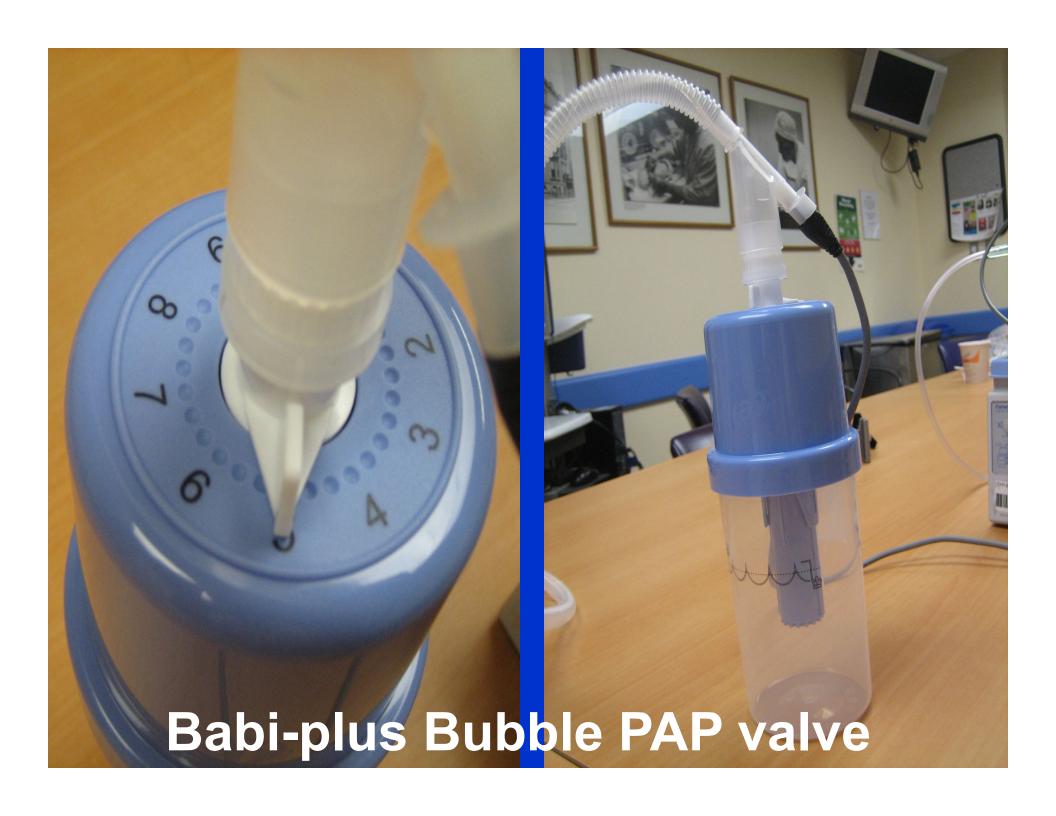



Bubble CPAP (Portable)



Nasal CPAP Application (6)

8. Choose the proper size of nasal Cannulae

CPAP Cannulae


Size	<u>B.W.</u>
0	< 700g
1	~1000g
2	~ 2000g
3	~ 3000g
4	~ 4000g
5	infant

Nasal CPAP



Secure tubings on both sides of the hat with either safety pins and rubber band or velcro

Nasal CPAP Application

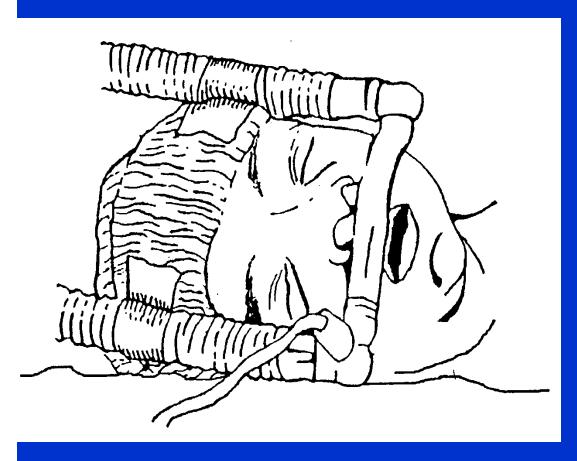


11. Secure tubings on both sides of the hat with either safety pins and rubber band or velcro










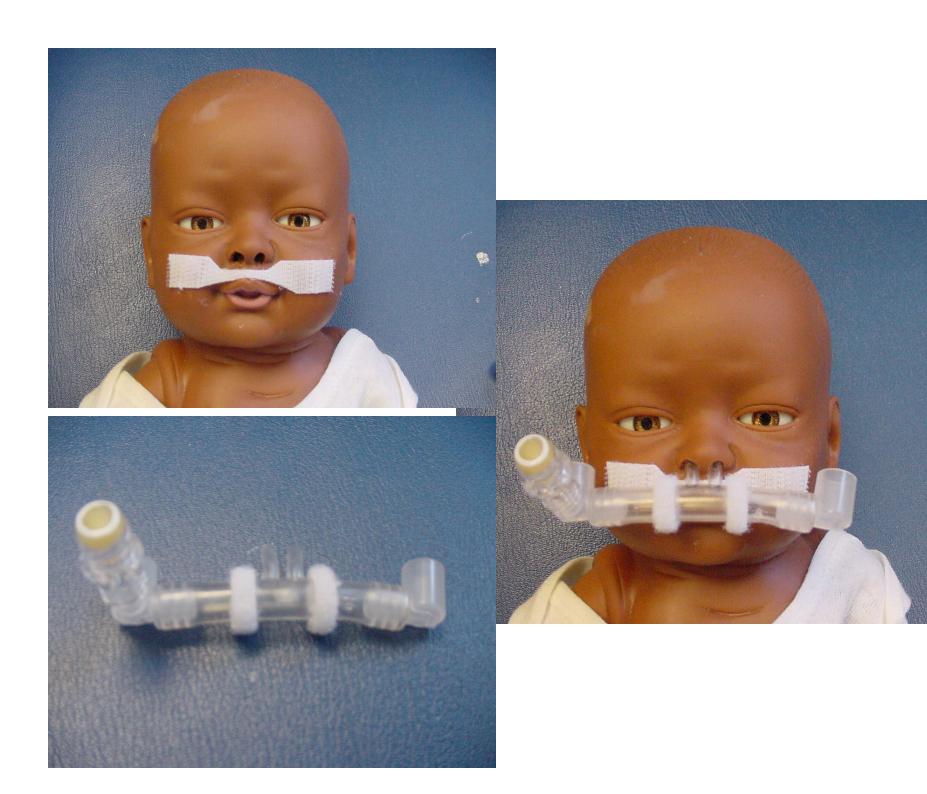


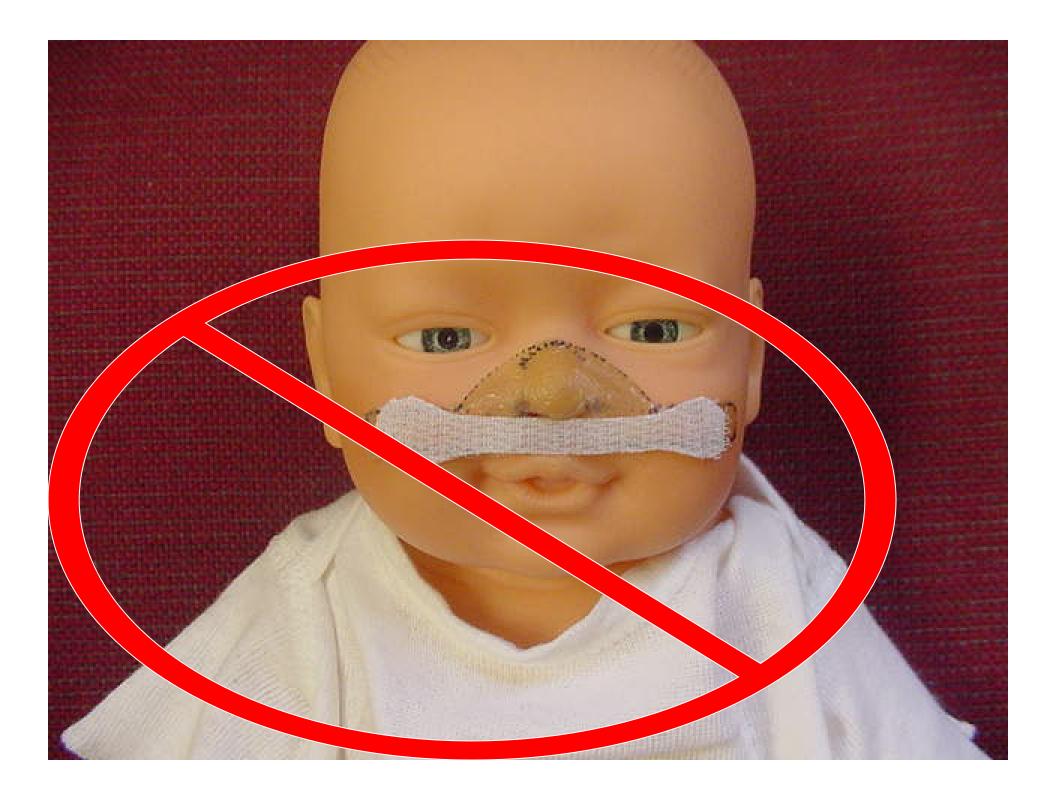








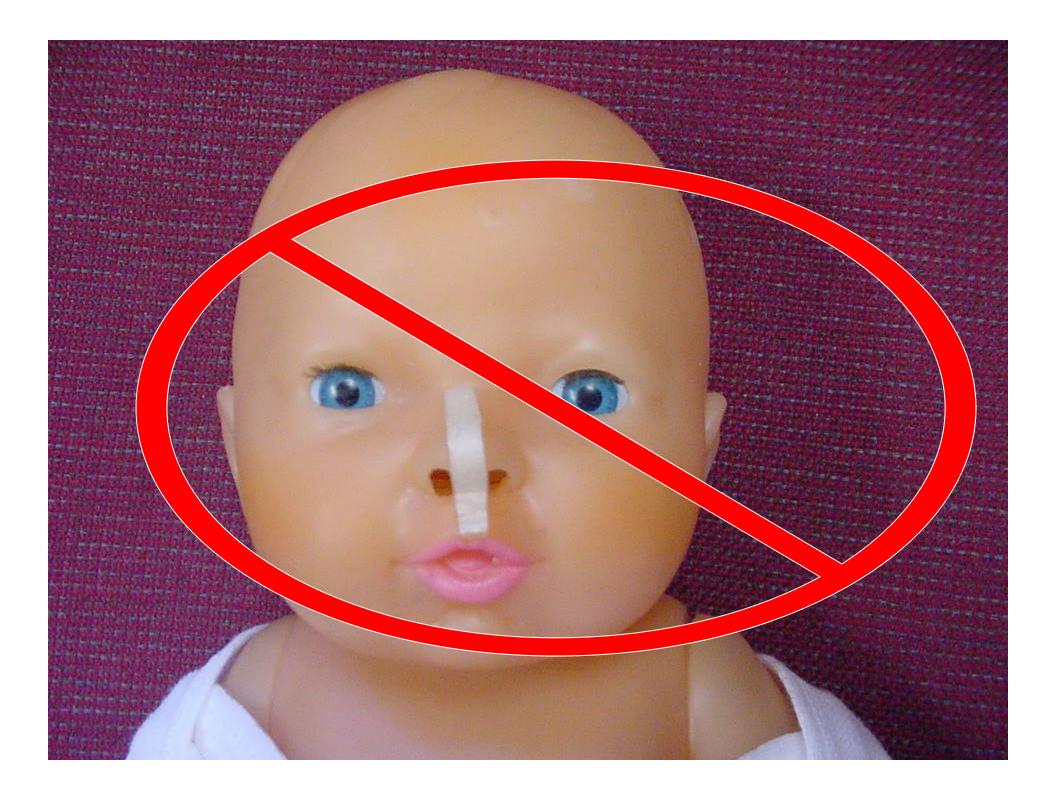

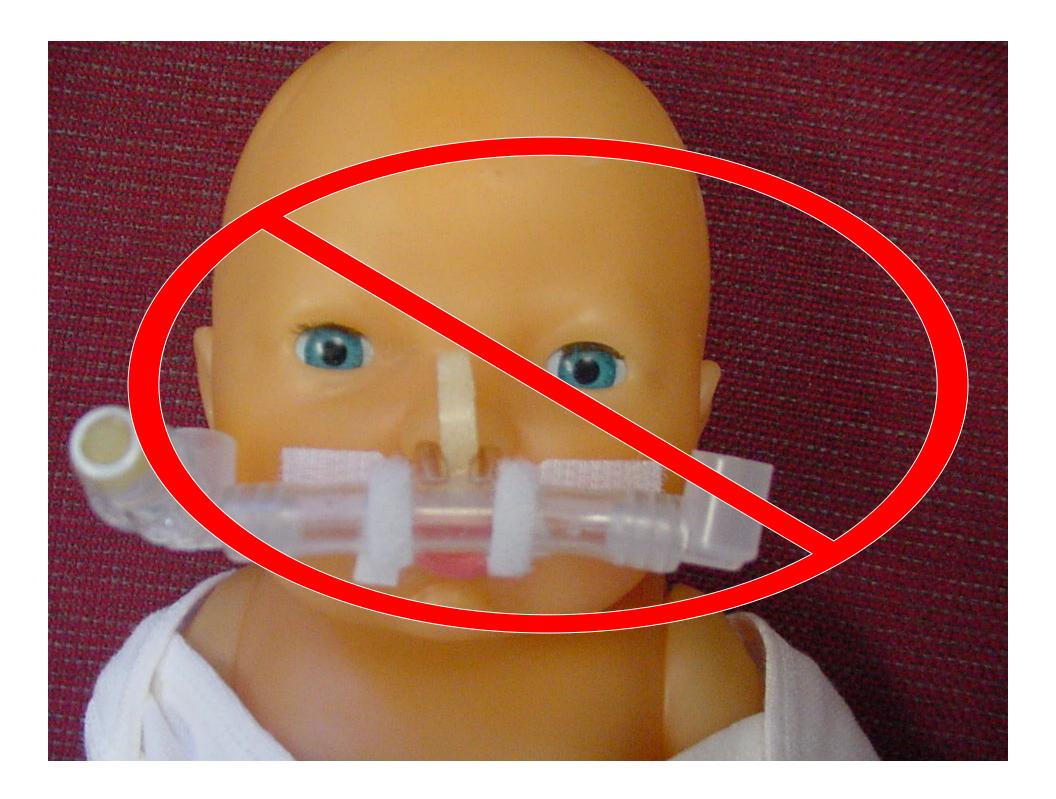


Pressure = Force / Surface Area









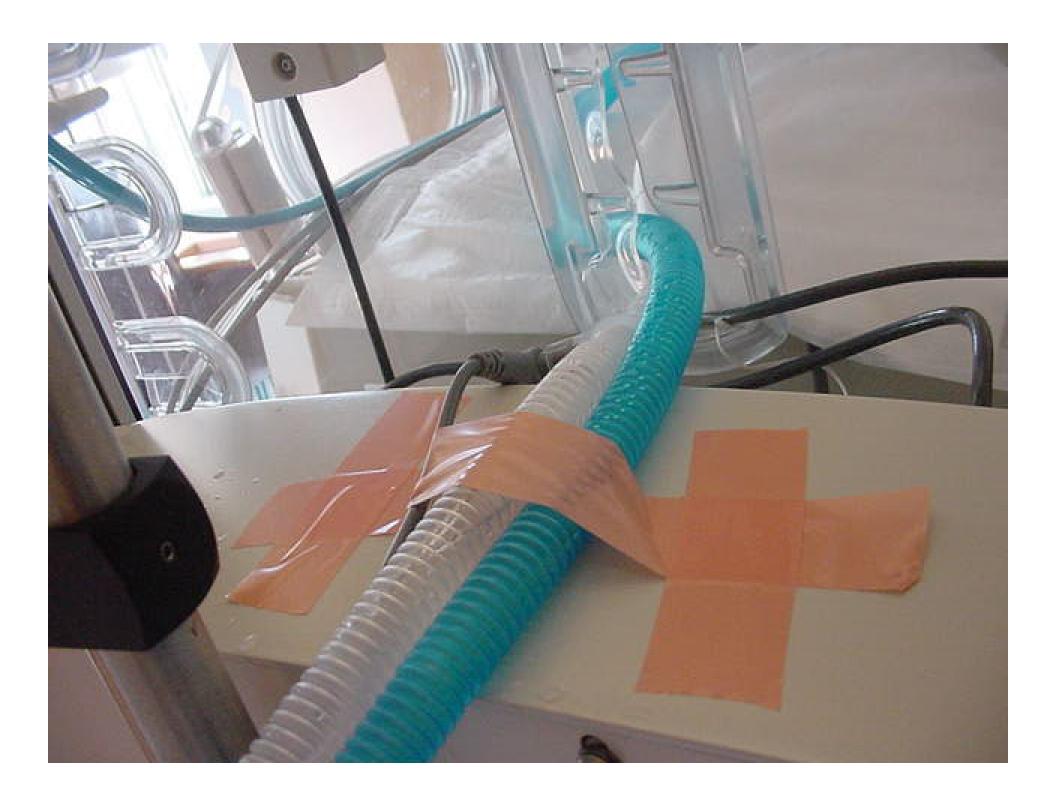

Nasal CPAP Maintenance (1)

- 1. Observe baby's vital signs, oxygenation and activity
- 2. Systematically check CPAP systems, inspired gas temperature, air bubbling out of acetic acid solution. Empty condensed water in the circuit
- 3. Check CPAP prongs position and keep <u>CPAP</u> cannulae off the septum at all times. A snug cap is used to securely hold the tubings in place and using self-adhesive Velcro to keep cannulae away from the septum if necessary

Nasal CPAP Maintenance (2)

- 4. Suction nasal cavities, mouth, pharynx and stomach q4h and prn
- 5. If baby swallows lot of air, insert gastric tube and suction should be more often.
- 6. Change the baby's position
- 7. Change CPAP circuit once a week

Nasal CPAP Weaning

- CPAP is kept at 5 cmH₂O
- FiO₂ is adjusted to keep PaO₂ in 50's, or oxygen saturation around 90% (alarm 85 -95%)

Nasal CPAP Discontinued

- No tachypnea or retraction
- No apnea and bradycardia
- FiO₂ is room air

Three CPAP weaning methods

- M1: Taken 'OFF' CPAP with the view to stay 'OFF'
- M2: Cycled on and off CPAP with incremental time 'OFF'.
- M3: As with M2, cycled on and off CPAP but during 'OFF' periods were supported by 2 mm nasal cannula at a flow of 0.5 l/min.

Arch Dis Child Fetal Neonatal Ed published online May 18, 2012

Methods of weaning preterm babies <30 weeks gestation off CPAP: a multicentre randomised controlled trial

	M1 (n=56)	m² (n=69)	M3 (n=52)	Sig
Time of wean‡	11.3±0.8	16.8±1.0	19.4±1.3	p<0.0001
Total days CPAP	24.4±0.1	38.6±0.1 [*]	30.5±0.1*	p<0.0001
CGA OFF CPAP	31.9±0.1	34.1±0.1	32.8±0.2	p<0.0001
Oxygen duration‡	24.1±1.5	45.8±2.2	34.1±2.0*	p<0.0001
BPD	7/56 (12.5%)	29/69 (42%)†	10/52 (19%)	p=0.011
Length of Admission	58.5±0.1	73.8±0.1 [*]	69.5±0.1*	p<0.0001
CGA at D/C#	35.8±0.1	36.9±0.1	36.9±0.1	p<0.0001

CGA: corrected GA;

Arch Dis Child Fetal Neonatal Ed published online May 18, 2012


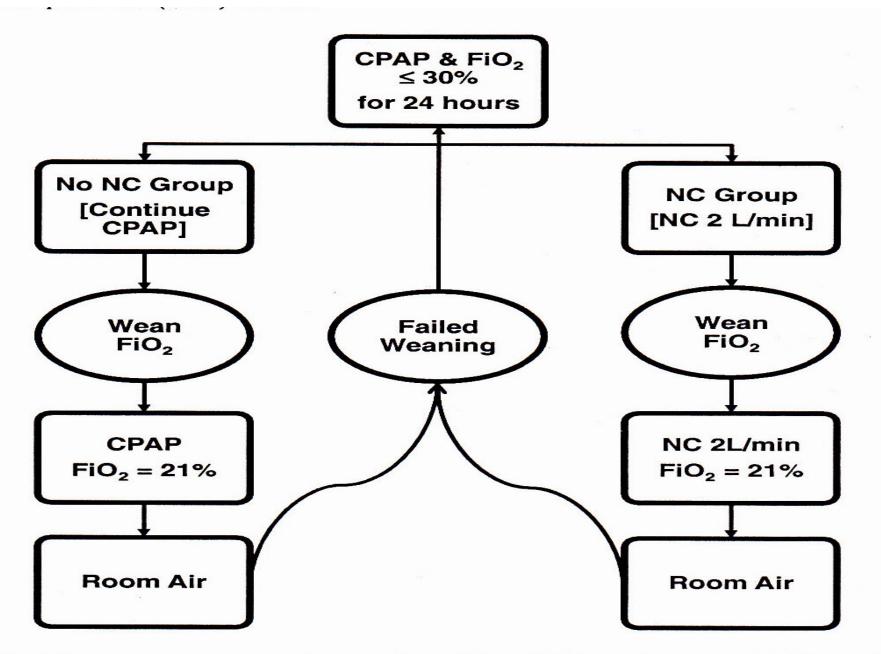


Fig. 1. Study design algorithm for weaning off NCPAP. NC: nasal cannula, NCPAP: nasal continuous positive airway pressure.

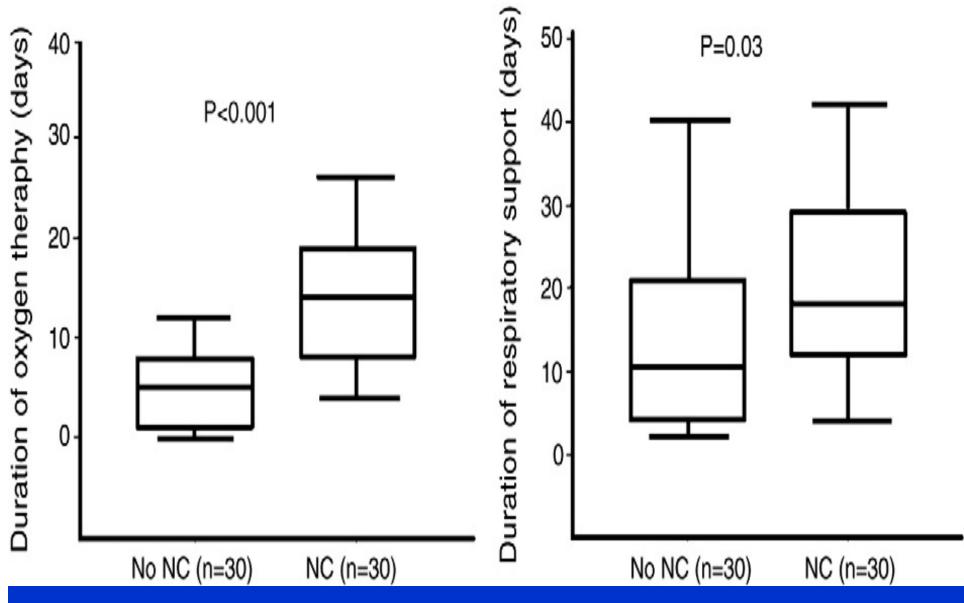

Duration of oxygen exposure and respiratory support in the two groups. Data are expressed in median and interquartile range. Mann–Whitney test was used.

Nasal CPAP Complications (1)

- Nasal obstruction from secretions or improper application of nasal prongs
- Gastric distention from swallowing air, abdominal distention, especially in infants on aminophylline or caffeine
- Nasal septum erosion or necrosis
- Fluctuating FiO₂
- Air leak: <5%, usually occurs during acute phase

Nasal CPAP Complications (2)

- Pneumothorax, if occurs, usually occurs within the first few days of use, not after a week. Furthermore, pneumothorax is generally less severe and less frequent in infants on CPAP compared to intubated infants on mechanical ventilation.
- Most of complications are preventable
- The majority of the problems can be attributed to inappropriate use, wrong device or a lack of training and experience





















Feeding on CPAP

Baby may feed at breast



Babies on NIV have adequate aerodigestive reflexes to prevent aspiration.

Concern over increased incidence of GERD is unfounded

Safety and efficacy of oral feeding in infants with BPD on nasal CPAP


Dysphagia. 2015 Apr. 30(2): 121-7


Hanin M, Nuyhakki S, Malkar MB, Jadeherla SR



CPAP Novel Application

- Mechanical ventilation via nasal CPAP cannulae
- Preferably in SIMV, A/C or pressure support mode. Infant Star Sync is not available anymore.
 - (using Servo I, N or U with NAVA).
- PIP: 15-20 cmH₂O, PEEP: 5 cmH₂O
- Indications:
- Frequent A&B
- ✓ High PaCO₂
- Laborious breathings

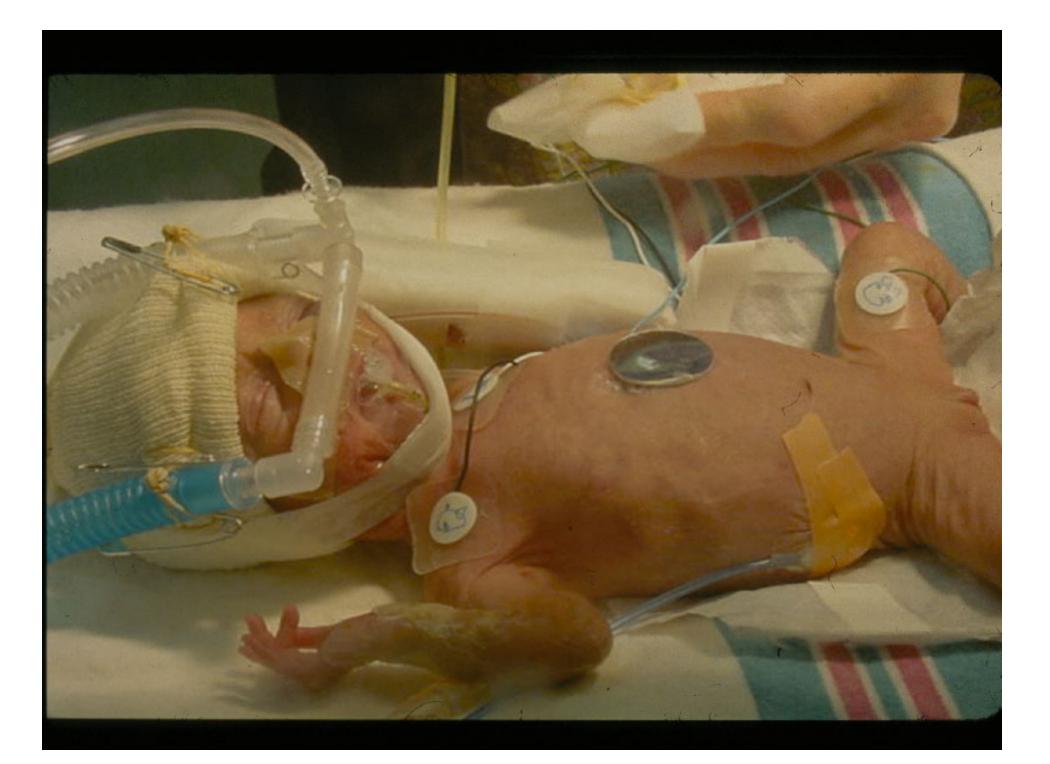

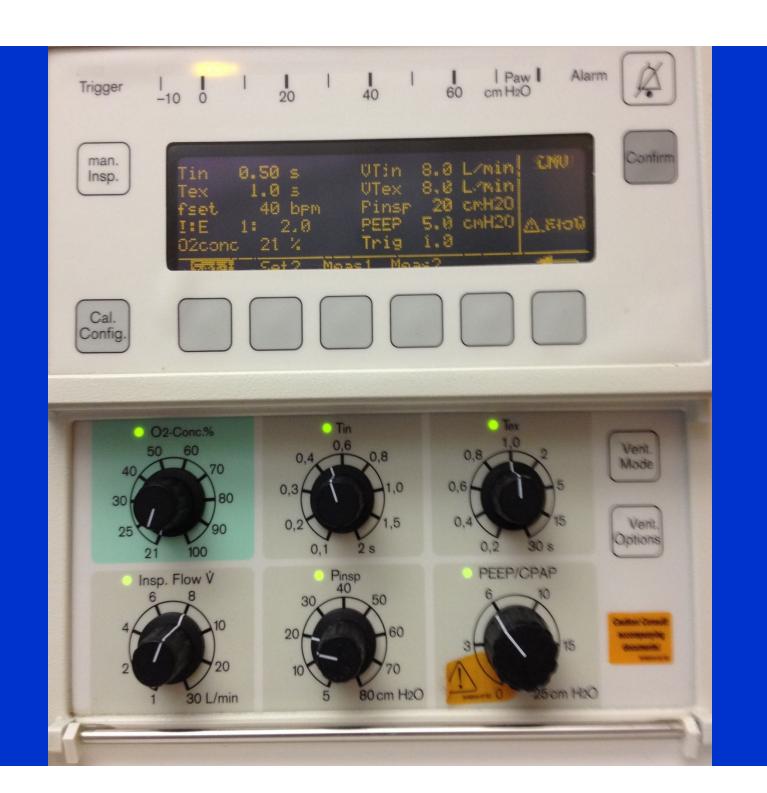




MAQUET GETINGE GROUP







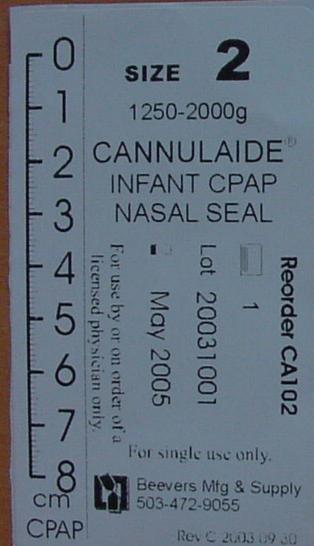





Mechanical Ventilation Indications

- 1.Marked retractions on CPAP (not due to nasal obstruction)
- 2. Frequent apnea and bradycardia on CPAP
- 3. $PaO_2 < 50 \text{ mm Hg with } FiO_2 > 60\%$
- 4. $PaCO_2 > 70 \text{ mm Hg (except } 1^{st} \text{ ABGS)}$
- 5. Intractable metabolic acidosis (BD > 10 meq/L after Rx with NaHCO₃)
- 6. Other (Cardiovascular collapse, Neuromuscular disorder, Congenital diaphragmatic hernia, or for Surgery, MRI, Cardiac catheterization, etc.)

The Columbia Experience with CPAP






The Columbia Experience (1997-1999)

A retrospective database review for a cohort of all live inborn VLBW infants (BW 500-1500g) born between Jan 1, 1997 and Dec 31, 1999 (three calendar years).

- 320 infants were divided into three groups:
- 1) <u>CPAP only group</u> (n = 230): received only bubble NCPAP for respiratory support during the first 24 hrs of life.
- 2) <u>CPAP failed group (n = 60)</u>: Infants managed initially with NCPAP who required intubation within 24 hrs of birth.
- 3) Vent only group (n = 30): Infants requiring intubation immediately following birth.

The Columbia Experience (1997-1999)

BW(gm)	CPAP	CPAP/	IMV	Total	Expired
	Only(%)	IMV(%)	(%)		(%)
500-750	21(31.8)	26(39.4)	19(28.8)	66	11(16.7)
751-1000	58(69)	17(20.2)	9(10.7)	84	6(7.1)
1001-1250	59(85.5)	9(13)	1(1.4)	69	0
1251-1500	92(91)	8(7.9)	1(1)	101	7(6.9)
Total	230(71.9)	60(18.8)	30(9.4)	320	24(7.5)

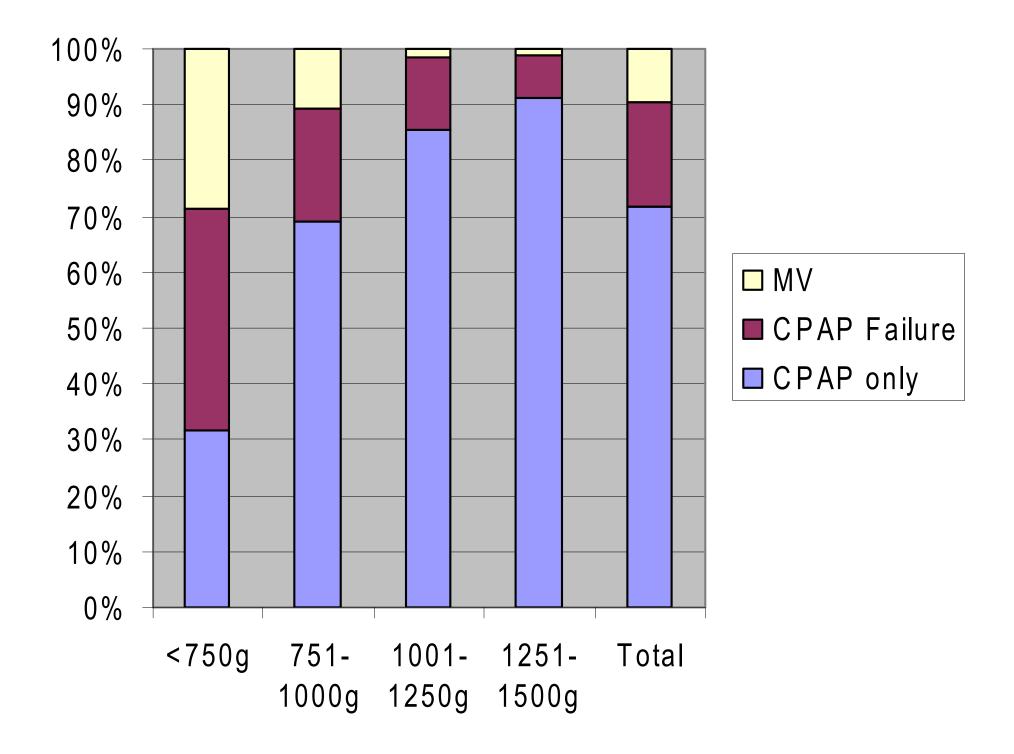

BPD (Required oxygen suplement at 36 wks PCA)

BW(gm)	CPAP only	CPAP/IMV	IMV	Total
500-750	0/21	1/26	3/19	4/66
751-1000	1/58	0/17	0/9	1/84
1001- 1250	0/59	0/9	0/1	0/69
1251- 1500	1/92	1/8	0/1	2/101

Intraventricular Hemorrhage (IVH Grade III-IV)

BW(gm)	CPAP only	CPAP/IMV	IMV	Total
500-750	1/21	3/26	4/19	8/66
751-1000	0/58	0/17	0/9	0/84
1001- 1250	1/59	0/9	0/1	1/69
1251- 1500	0/92	1/8	0/1	1/101

Retinopathy of Prematurity (ROP Stage 3-4)

BW(gm)	CPAP only	CPAP/IMV	IMV	Total
500-750	4/21	5/26	3/19	12/66
751-1000	0/58	0/17	0/9	0/84
1001- 1250	0/59	0/9	0/1	0/69
1251- 1500	0/92	0/8	0/1	0/101

Mortality before Discharge

BW(gm)	CPAP only	CPAP/IMV	IMV	Total
500-750	0/21	3/26	8/19	11/66
751-1000	1/58	3/17	2/9	6/84
1001- 1250	0/59	0/9	0/1	0/69
1251- 1500	3/92	3/8	1/1	7/101

The strategy of

Early nasal CPAP therapy first and

Surfactant replacement only for rescue

does not jeopardize outcome of very low birth weight infants


- Question: is the prophylactic administration of surfactant superior to early rescue treatment in spontaneously breathing infants supported on nCPAP, in reducing the need for mechanical ventilation, during the first 5 days of life?
- Population: 25-28 weeks infants (European multicentre, n=24)

• Outcome:

- . Duration of mechanical ventilation during the first 5 days of life
- . Mortality, pulmonary and neurological morbidity



CURPAP study: method

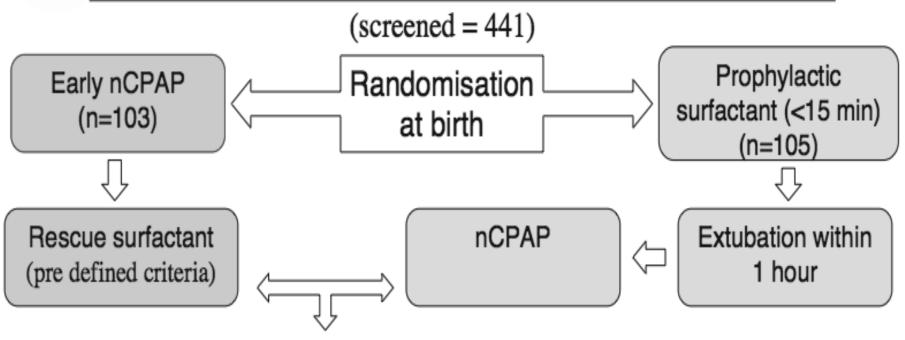

CPAP failure = intubation FiO2 > 0.40 PaCO2 > 65mmHg

CURPAP study: preliminary results

Parameter	nCPAP	CURPAP
Gestational age (median in weeks)	27	27
Birth weight (g)	913 <u>+</u> 200	967 <u>+</u> 221
Antenatal steroids	98%	96%
CPAP failure => mechanical ventilation	31%	33%
Pneumothorax	1%	6.7%*
Mortality	10.7%	8.6%
BPD	22%	23.8%

50% resources

50% rescue surfactant (median =240 min of age)




Summary of the CURPAP study

- Prophylactic surfactant is <u>not</u> superior to early rescue surfactant therapy after CPAP
- Surfactant was halved in the nCPAP group
- Outcome was really good in both arms

NICU Quality and Outcome, 2013 501 - 1500g

	MSCH (Columbia)	Vermont Oxford
Incidence of BPD	7.7%	34.6%
Nosocomial infection	5.8%	13.4%
Incidence of IVH	13.5%	25.9%
Incidence of Severe ROP	6.3%	7.8%
Incidence of NEC	5.5%	6.7%
Neonatal Mortality rate	9.5%	15.0%

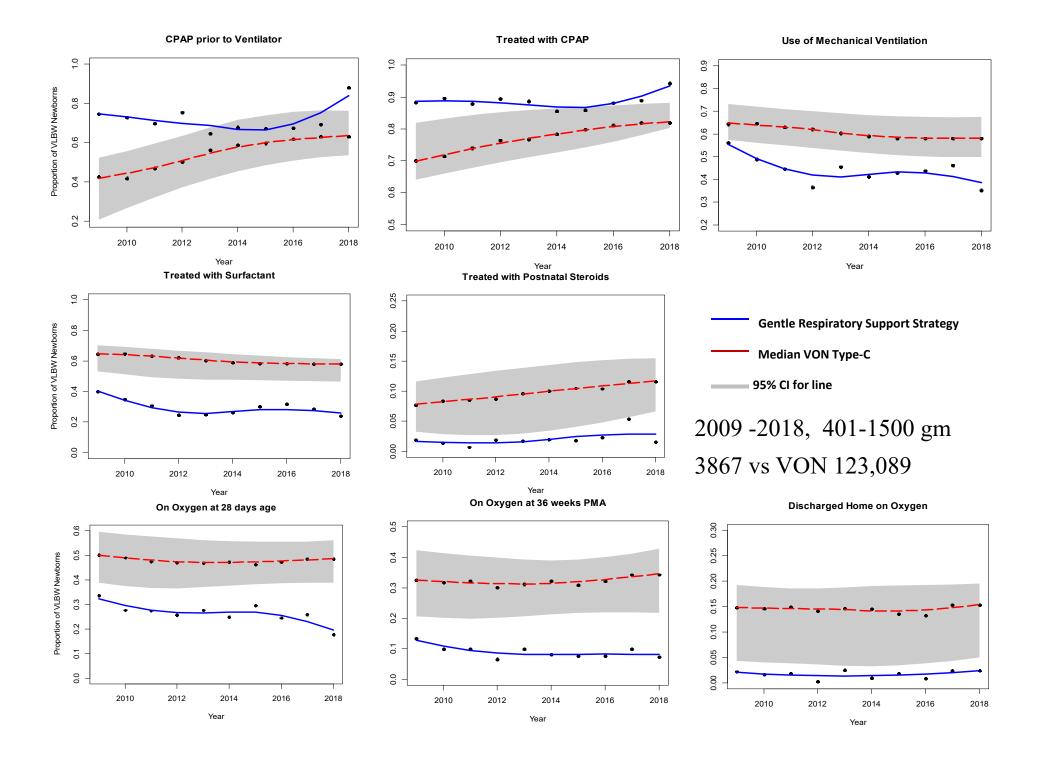

Do not brand a form of therapy as useless,

when in reality it was only inappropriately applied.






Key strategies for the successful use of nasal CPAP therapy

- 1. Choose the right bubble nasal CPAP device and interface
- 2. Familiarize caregivers with the device
- 3. Learn to use nasal CPAP correctly, gain experience, increase in the comfort level of Staff and it takes a village
- 4. Initiate nasal CPAP early. No weight limit
- 5. Maintain nasal CPAP with meticulous airway care & pay attention to details
- 6.Tolerate PaCO₂ up to 60's mmHg & FiO₂ up to 60%
- 7. Extended use of nasal CPAP till on room air without respiratory distress to enhance the growth of the premature lung



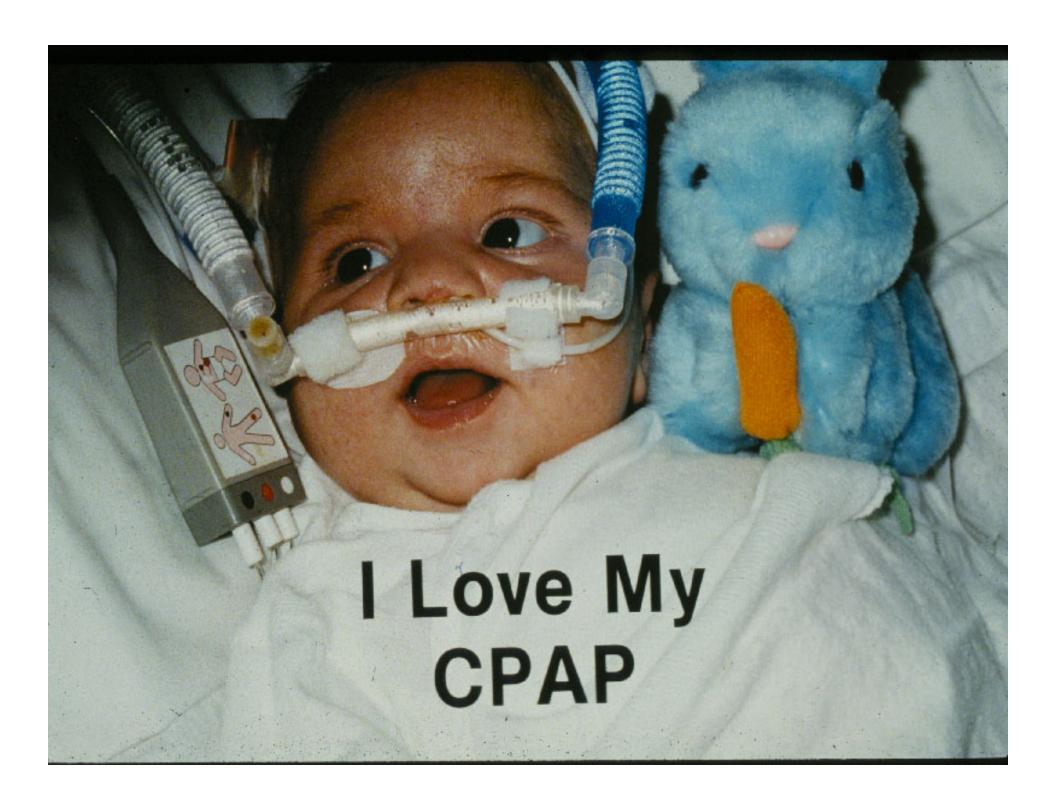



1)There are following three CPAP weaning methods. Which is the preferred method?

Answer: a

- a) Off CPAP when the infant is stable on room air without respiratory distress. Resume CPAP if tachypnea, retraction or requires oxygen supplement
- b) Cycled on and off CPAP with incremental time 'OFF'
- c) Cycled on and off CPAP, but during 'OFF' periods were supported by 2 mm nasal cannula at a flow of 0.5 l/min.

2) Use of HFNC vs CPAP in ELBW infants. HFNC is associated with the followings, except:

Answer: c

- a) A higher risk of death or BPD
- b) Increased respiratory morbidities
- c) Early oral feeding
- d) Prolonged hospitalization.